Bayer HealthCare

Instructions for programming maximum flow rate with Continuum

To access the adjustable settings:

1. Press the **INFO** button twice.
2. Scroll to “Adjust Setting”, then press **START/OK.**

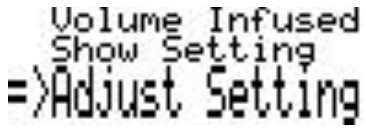

3. Scroll to “More…” then press **START/OK.**
4. Enter Code 901 then press **START/OK.**
5. Scroll to “Maximum Flow Rate”, then press **START/OK.**



6. Enter the rate and press **START/OK.**
7. Rate should be set at 500 ml/hr.
8. When done, choose **Restart Pump** from the menu.
9. Confirm that the correct Maximum flow rate has been entered:

   The Show Setting feature is designed to allow you to view the programmable options and other important information about the pump. In Show Setting, the current settings can be viewed, but cannot be changed.

10. Press **INFO** twice. The screen below is displayed



MEDRAD, INC.

100 Global View Drive
Warrendale, PA 15086
U.S.A.

(412) 767-2400

www.ri.bayer.com

11. Press the **DOWN ARROW** button to select Show Setting. Press **START/OK** and the current settings are displayed, but cannot be changed. To view the setting for a particular option, select the desired option, then press **START/OK.**
12. Maximum flow rate should be set at 500 ml/hr.